

APPENDIX 2

FIGURE 3

The Danish version of the Stop-Bang Questionnaire measured receiver's operating characteristic curve for Apnoea Hypopnoea Index values > 5.

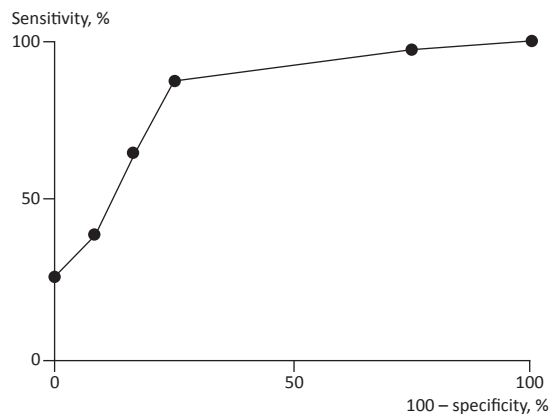


FIGURE 5

The Danish version of the Stop-Bang Questionnaire measured receiver's operating characteristic curve for Apnoea Hypopnoea Index values > 30.

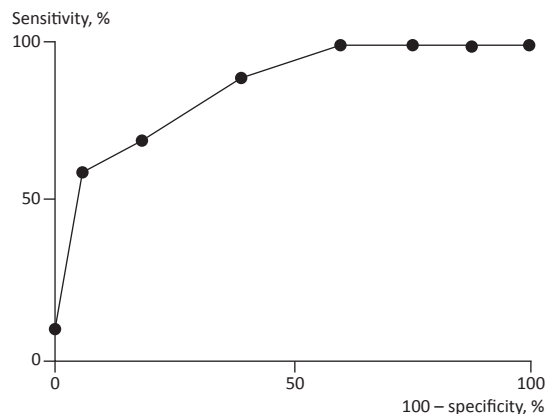


FIGURE 4

The Danish version of the Stop-Bang Questionnaire measured receiver's operating characteristic curve for Apnoea Hypopnoea Index values > 15.

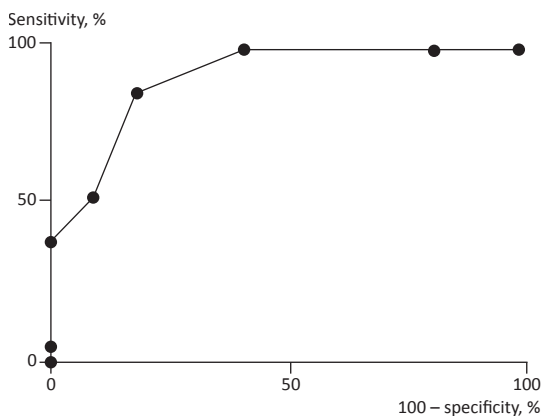


TABLE 3

Characteristics of the Danish version of the Stop-Bang Questionnaire scores with a test cut-off value of 5.

	AHI > 5	AHI > 15	AHI > 30
Patients, n	17	16	7
Sensitivity, %, median (95% CI)	64.5 (45.4-80.8)	85.7 (63.7-97.0)	90 (55.5-99.8)
Specificity, %, median (95% CI)	83.3 (62.6-95.3)	81.8 (59.7-94.8)	60.6 (42.1-77.1)

AHI = Apnoea Hypopnoea Index; CI = confidence interval.